

# Digital Bandwidth Interleaving

Peter J. Pupalaikis  
Principal Technologist  
March 29, 2005

"The number of transistors on a chip doubles every 18 months."


- attributed to Gordon Moore  
Co-founder Intel Corp.

The empirical and eponymous Moore's Law<sup>1</sup> claims that transistor density doubles every 18 months. Since transistor speed is roughly proportional to linear density, it implies that transistor speeds double every three years. Since the oscilloscope, while undergoing many changes during its long history, is still the primary tool used in the development of electronic instruments, Moore's law dictates that the available oscilloscope bandwidth must also double every three years in order to keep pace.

With regard to the real-time oscilloscopes (equivalent time, or sampling oscilloscopes have different rules), bandwidth increases of late have traditionally come through the utilization of higher speed processes in the design and development of oscilloscope front-end amplifiers, ADCs and memories. Unfortunately for the oscilloscope manufacturers, this means the redesign of various custom ICs, with costs increasing at an exponential rate.<sup>2</sup> As the life-cycle of these high performance instruments continues to shrink, these costs are passed on to oscilloscope customers.

Historically, wise companies realize that the trends dictated by Moore's Law only perpetuate the problem. Oscilloscope manufacturers continue to march along the curve of inexorable bandwidth increases, bearing the pain of these increases. But throughout history, companies have occasionally found breakthrough

innovations that change the so called rules. There are many examples of such feats. Perhaps one of the best examples is found by examining the history of the hard-disk drive and the invention of PRML, which enable densities that far exceeded the predictions of the governing trends.<sup>3</sup>

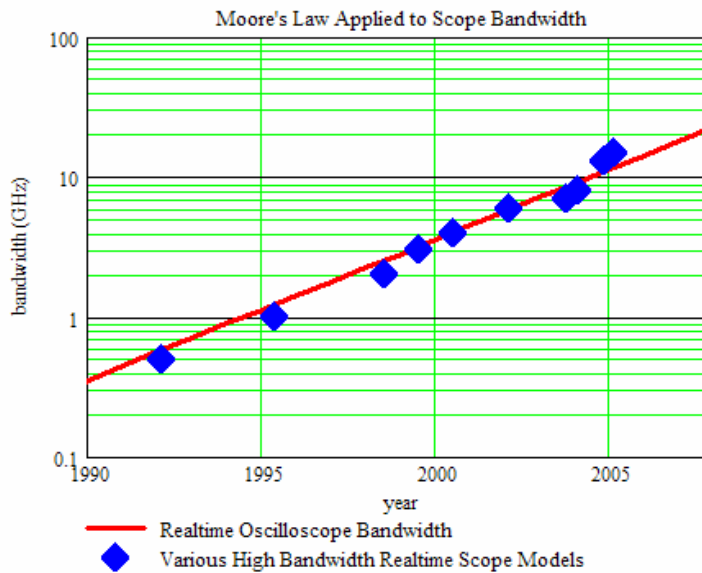

In the area of high bandwidth oscilloscope design, the major innovation that has been carrying the industry for the last two decades is that of *interleaving*. Interleaving is the combination of channel resources, namely the channel digitizers and memory, to create oscilloscopes with very high sample rates and memory lengths. This innovation relieves constraints on individual


digitizer speeds that are far below the effective sample rates achieved. While interleaving has been highly successful, it does not address bandwidth, since Interleaved digitizers are driven by a front-end amplifier which must be designed to accommodate the end bandwidth of the instrument.

LeCroy has developed a new interleaving technique called *Digital Bandwidth Interleave* - or DBI - which provides the same benefits for increasing sample rate and memory length as traditional techniques, but allows for increasing bandwidth as well.

While traditional interleaving has certain hardware requirements of delivering signals and clocks to multiple paths, the problem is mainly calibration of the timing and gain/offset of the multiple paths. There are many ways to approach this calibration, and the algorithms for obtaining the best correction can be quite complex. However, the software which accomplishes the interleave is basically straightforward.

Digital bandwidth interleave, on the other hand, involves additional hardware, calibration and digital signal processing at the back end to recover the signal input by the oscilloscope user.

A simplified diagram of the hardware topology of DBI is shown. Basically, the input signal is split with a diplexer. A diplexer is a microwave filter designed to split incoming signals into multiple frequency bands. In the case of a two channel, bandwidth doubling arrangement, the low frequency band is delivered from the diplexer directly into one front end. The cutoff of the low frequency path from the diplexer has been designed to pass an entire frequency band which meets the bandwidth capabilities of the oscilloscope front-end. The high frequency band enters a downconverter. The downconverter is realized utilizing a wide-band mixer. The downconverter mixes a predetermined local oscillator with the incoming high frequency band and produces two image bands – one at the difference frequency and the other at the sum frequency. The difference frequency is an image of the high frequency band passed to the mixer, but is now within a band that can be handled by the oscilloscope front-end. Therefore the high frequency band has been shifted in its entirety to a lower frequency band. This uses the same basic concept as a radio receiver. In essence, both the low and high frequency bands are acquired by the

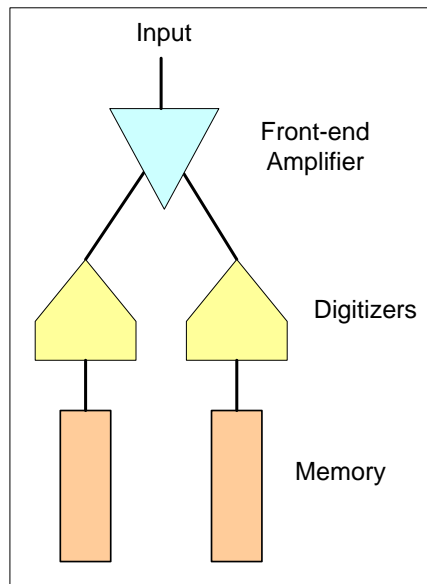


**Traditional Interleave Topology**

oscilloscope, with the low band in its original location and the high band "moved" to a different (lower) frequency location.

Once acquired, each band undergoes signal processing. The main effect of the processing is to remix the high frequency band with a digitally synthesized replica of the local oscillator to move the band into the correct frequency locations. It also digitally rejects the new image created by the mixing action. Finally, the two bands are recombined forming an acquisition that is almost double the bandwidth of an acquisition utilizing a single oscilloscope channel.

A key point to remember about DBI is that each frequency band is within the bandwidth capability of the acquisition channel which will acquire it. The digital signal processing is used to recombine the waveforms, but is not being used to "extend" the bandwidth of a channel. Thus, the problems with bandwidth extension, such as increased noise, are not introduced in a DBI based oscilloscope.

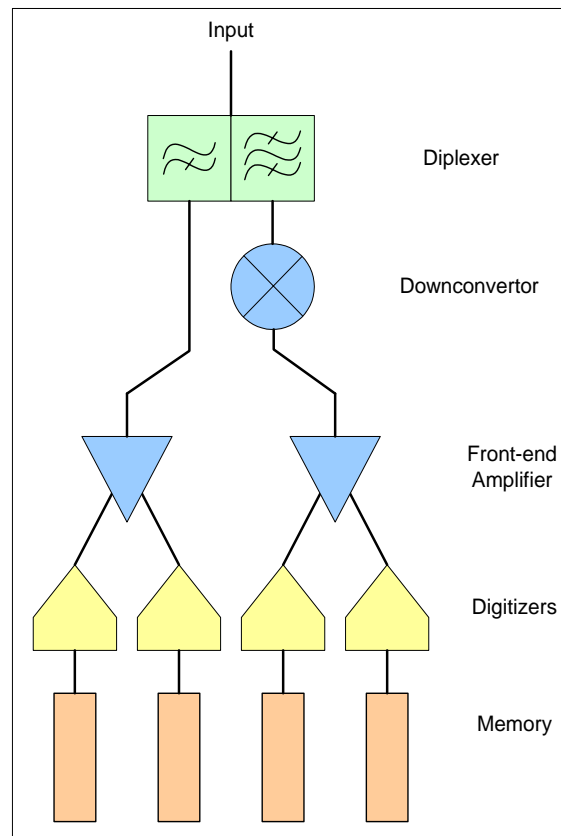

**Bandwidth Interleave Topology**

DBI technology is enabled by two key elements: The first is the recent improvements in the performance of microwave and RF technologies. A new generation of wide bandwidth amplifiers, mixers, attenuators, filters, etc. can achieve the amplitude accuracies required for use in the input signal path of a real time oscilloscope.

The second enabler is the speed of digital signal processing within Intel Pentium processor based instruments. While not generally thought of as a "signal processor", the Pentium is the fastest floating point digital signal processor in the world<sup>4</sup>.

With the available raw processing power, LeCroy mastered the digital signal processing techniques for the compensation of analog signal paths. The final challenge was

devising and implementing the complex routines used in the automated test systems which calibrate the instrument. The result is a solution that operates with incredible performance.

DBI is a technology that shifts the limitations on real-time oscilloscope bandwidth from cost, design effort and speed limitations of IC design processes available to limitations dictated by speeds of RF and microwave design technology. As applied today, DBI lifts the bar by at least a factor of three and will continue to increase in the future.

As such, DBI is an innovation that provides a discontinuity or disruption in the oscilloscope bandwidth trend. In the future, LeCroy will introduce oscilloscopes with DBI built in at the beginning of the design cycle. Future realtime oscilloscopes will give the user the ability to eliminate bandwidth as a prime consideration when trying to determine which types of instruments will suit their measurement needs.

The resulting DBI enabled oscilloscope performs the same as an instrument implemented with traditional technology. Parameters such as accuracy and noise are essentially the same. Frequency response accuracy and return loss, parameters of particular importance for accurately reproducing eye diagrams of serial data signals, have actually improved in the first instrument designed with DBI.



**The SDA 11000 – LeCroy’s first DBI enabled serial data analyzer operates at 11 GHz bandwidth and 40 GS/s sample-rate**


*The author is Principal Technologist at LeCroy and a co-inventor of the Digital Bandwidth Interleave technology. He has held a variety of titles during his ten year career at LeCroy including digital signal processing engineer and product marketing manager for high performance oscilloscopes. He holds a BSEE from Rutgers University and is a member of Tau Beta Pi, Eta Kappa Nu and the IEEE communications and signal processing societies. He holds several patents in the area of the application of digital signal processing to measurement instruments.*

<sup>1</sup>Gordon E. Moore, “Cramming more components onto integrated circuits”, Electronics, Volume 38, Number 8, April 19, 1965

<sup>2</sup>Simon Young, “The Risk/Reward Realities of Chip Development”, TechOnLine Publication, Nov. 7, 2002

<sup>3</sup>Clayton M. Christensen, “The Innovator’s Dilemma”, Harvard Business School Press, 1997

<sup>4</sup>BDTImark2000™ Scores, Berkeley Design Technology, Inc., June 2001

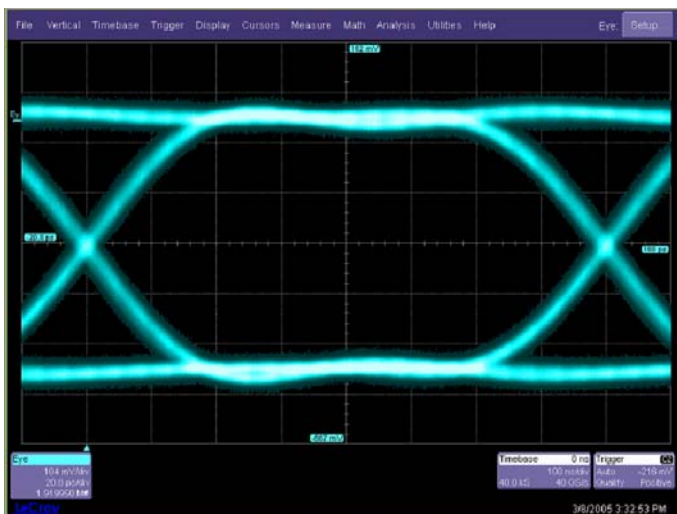

**Eye pattern from 6 Gb/s PRBS measured with SDA 11000**



**1-800-5-LeCroy**  
**www.lecroy.com**